


**MEDICA Pro 30/60/120**

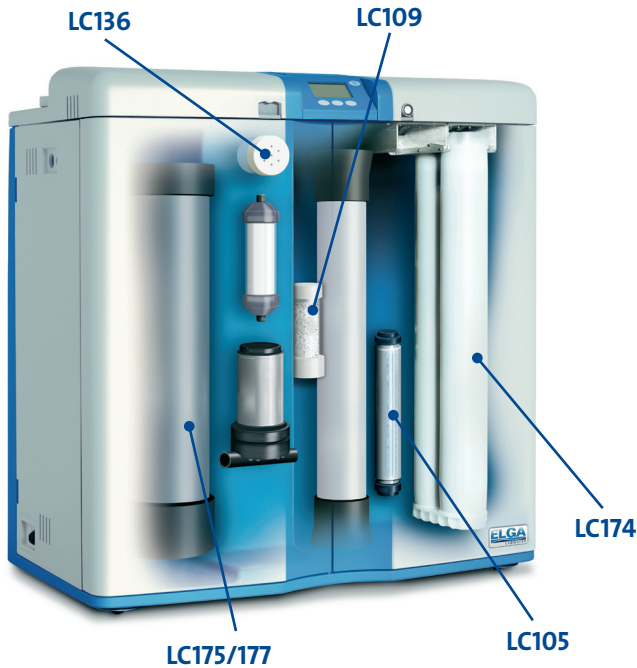

| Consumables               | Typical replacement intervals |
|---------------------------|-------------------------------|
| LC105 (UV lamp)           | 12 months                     |
| LC175 (Protek L1)         | 6 months                      |
| LC177 (Protek L2)         | 12 months                     |
| LC109 (UMF cartridge)     | 12 months                     |
| LC174 (Medpure L1)        | Maximum 12 months             |
| LC136 (Bacterial filter)  | 6 months                      |
| CT3 (Disinfection tablet) | 6 tablets per month           |

| Display id | Icon            | Alarm                              |
|------------|-----------------|------------------------------------|
| 672-99     |                 | Low voltage                        |
| 672-98     |                 | Leak detection                     |
| 672-97     |                 | Reservoir level controls           |
| 672-96     |                 | High loop pressure                 |
| 672-95     |                 | Permeate over temperature          |
| 672-94     |                 | Delivery loop over temperature     |
| *** - 93   | <br>LC175/LC177 | Protek L1/L2 incorrectly installed |


| Display id | Icon         | Alarm                            |
|------------|--------------|----------------------------------|
| *** - 92   | <br>LC174    | Medpure L1 incorrectly installed |
| *** - 90   | <br>10 MΩ-cm | Water purity alarm               |
| *** - 89   | <br>35°C     | Water temperature alarm          |
| *** - 88   | <br>30 μS/cm | Permeate purity alarm            |
| *** - 87   | <br>35°C     | Permeate temperature alarm       |
| *** - 86   |              | Break tank low                   |
| *** - 85   |              | UV lamp fail                     |

**MEDICA Pro 30/60/120**


**RO DISINFECTION**

PRESENT GREEN disinfection key to reader.

PRESS ✓ to enter the disinfection options.




PRESS ✓ to enter RO disinfection.




UNSCREW the large white lid on the right of the unit.

Add 2 CT3 tablets.  
Replace lid.







PRESENT GREEN disinfection key to confirm that the chemical has been added.



The unit will now complete the remainder of the cycle automatically.

This cycle lasts approximately 1 hour.

Once the water quality has been flushed below the alarm set point the unit will complete disinfection.



PRESS ✓ to accept the sanitization reminder.



**EMERGENCY BYPASS**

Contact your local service provider before putting the unit into emergency bypass.



**MEDICA Pro-R/RE/RX**

- Ensure the process is OFF
- Disconnect the electrical supply.
- Open the doors.
- Close valve 1.
- Close valve 2.
- Remove yellow plastic cover 3.
- Open valve 3.
- Close valve 3 when there is no requirement for purified water.
- Monitor water purity independently or install new Medpure L1 cartridges to guarantee water purity.

**MEDICA Pro-B/S/SE**

- Ensure the process is OFF.
- Disconnect the electrical supply.
- Open the doors.
- Close valve 1.
- Valve 2 should remain closed.
- Remove yellow plastic cover 3.
- Open valve 3.
- Monitor the level in the reservoir to ensure it does not overflow.
- Monitor water purity independently or install new Medpure L1 cartridges to guarantee water purity.
- Close valve 3 when there is no requirement for purified water.